


Vestibular Function Testing

Timothy C. Hain, MD

Vestibular Tests

- ENG (electronystagmography)
- VEMP (Vestibular evoked myogenic responses)
- Rotatory Chair
- Posturography

Five motion sensors – can measure two

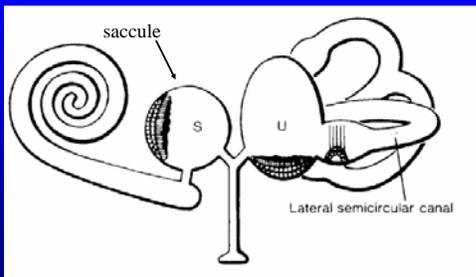

Schematic of Inner Ear (Frenzel, 1955)

What are we testing?

- VOR (i.e. input/output, ENG/Rchair)
 - Lateral canal only
- VCR (VEMP test)
 - Saccule only
- Abnormal gravity sensitivity (positional nystagmus)
 - BPPV
- Central tracking and visual acuity (pursuit, saccade test, OKN test)
- Sensorimotor integration (posturography)
 - Documents something related to balance
 - Diagnoses Malingering

Believe in yourself ! (your own exam)

- Quality control on vestibular testing is nonexistent
- Computer software is crude
- No method exists of recording torsion (which you need for BPPV)
- There are many places where corners can be cut or things can go wrong
- Experienced eyes (with Frenzels) are far more reliable than most ENG's.



Electronystagmography (ENG or VENG) consists of a battery

- Calibration test (saccades)
- Spontaneous nystagmus test
- Oscillating tracking tests (Pursuit)
- Positional tests (Hallpike)
- Caloric test



Calibration Test

- Calibration (of course)
- Gaze-evoked nystagmus (cerebellar)
- Saccades
 - Oculomotor disorder
 - Gaze palsy
 - INO
 - Cerebellar disorder
 - Overshoot and undershoot




Calibration test: Bottom Line

- Can detect cerebellar disorders and oculomotor palsies (which are rare).
- Unreliable (i.e. not sensitive)
- Often misinterpreted
- Your eyes (bedside exam) are usually more accurate.

Spontaneous Nystagmus Test


- Record nystagmus in light and dark
 - Acute vestibular disorders have strong horizontal “jerk” nystagmus.
 - Normal people and chronic vestibular disorders have little or no nystagmus. Neural compensation for vestibular tone asymmetry is fast and effective. Most people can’t “fake” nystagmus.
 - Almost everything unusual is central.

No spontaneous nystagmus (Normal)

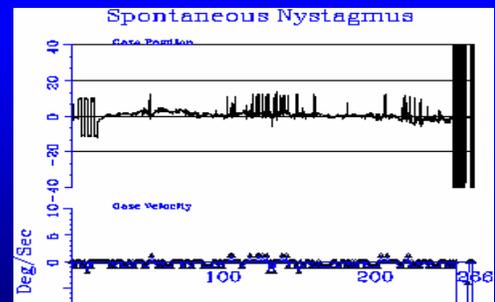

Up to 2 deg/sec of SN is normal for IR, 5 deg/sec for EOG

Vestibular Spontaneous Nystagmus (slightly abnormal)

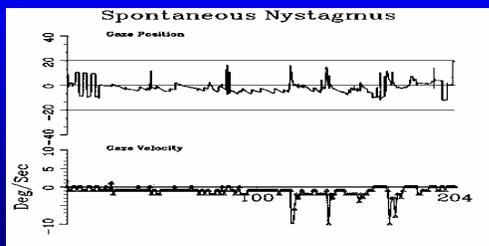

Vestibular Spontaneous Nystagmus (very abnormal, temporal bone fracture, dizzy and deaf)




Spontaneous Nystagmus Test: Bottom Line

- If present, very useful because documents that there is either a acute vestibular disorder or central problem.
- If not present, not helpful. Disorder may be intermittent or chronic (SN goes away).
- Your own eyes (with video Frenzels) are more accurate than ENG

Oscillating Tracking Test Smooth Pursuit is impaired by:

- Central disturbances -- most cause a transient disturbance only.
- Medications
- Age

Normal oscillating tracking test (Smooth Pursuit)

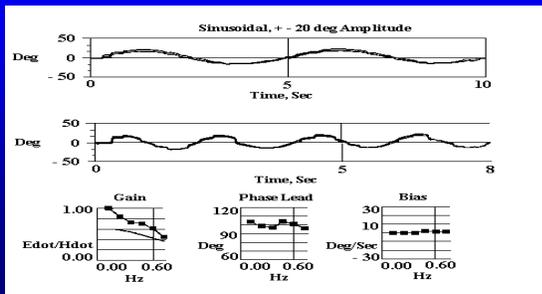


Pursuit Test: Bottom line

- Smooth pursuit testing is rarely useful for clinical diagnosis.
- No implications for PT either

Positional/Positioning Testing

- Hallpike test for BPPV (common condition). No ENG torsion measure – your eyes are better !
- Positional test for non-BPPV positional nystagmus. These are extremely rare, however.
- Central positional nystagmus


Posterior canal BPPV (R)

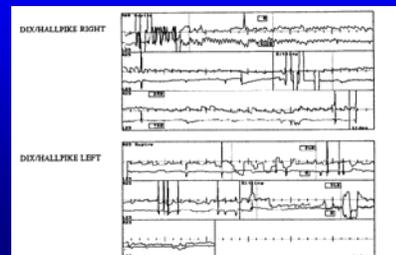

What the ENG people see on VNG (hard to see torsion too)



Lateral Canal BPPV (R)

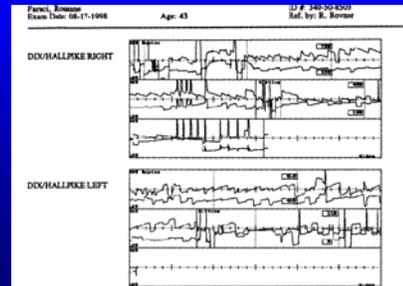

Central Positional Nystagmus

- Anything is possible (can resemble BPPV and variants closely)
- DBN supine most common
- UBN next most common
- Generally no PT intervention will work (but worth a try anyway)

Positional Testing Bottom Line


- Positional testing is useful to diagnose classic BPPV and variant BPPV (20% of all dizziness)
- Your own eyes with Frenzels is better than ENG in most instances
- Assume any ENG positional is BPPV until you exhaust treatment

Caloric Testing – unilateral weakness: Method


- Hot and cold water in ear (a little messy)
 - Some labs use air – not a good idea
 - Some labs use balloons – not a good idea either
- Measure nystagmus
- Compare ears and total nystagmus



Measure Nystagmus induced by warm or cold water

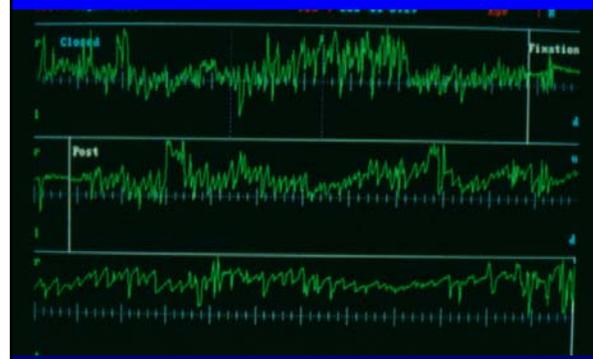

Normal Caloric

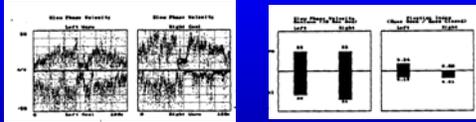

Unilateral Weakness 5.5 % Left
 Directional Preponderance 5.3 % Left
 Total Response 100.5 deg/sec
 Spontaneous Nystagmus 1.2 deg/sec Left
 Results Corrected for Spontaneous Nystagmus

$100 * (RC + RW - LC - LW) / (RC + RW + LC + LW)$
 $100 * (RC + LW - RW - LC) / (RC + RW + LC + LW)$
 $(RC + RW + LC + LW)$

Caloric Testing


- **Paresis** compares one side to the other. Up to about 30% is OK, but takes some judgement. Most useful measurement.
- **Total response** compares all four responses to norms. Greater than 20 deg/sec is normal. Useful if water is used, useless if air is used

Caloric Testing Bottom Line


- Definitive method of diagnosing a unilateral vestibular lesion.
- Calorics are the only thing you can't easily do yourself (with Frenzels)
- You can do spontaneous, HSN and Vibration though (which are pretty good)

VEMP testing

- Exciting new test – of VCR
- Loud clicks in one ear
- Record from SCM

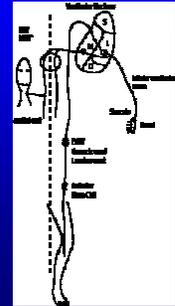


Abnormal VEMP in Vestibular neuritis (absent one side)

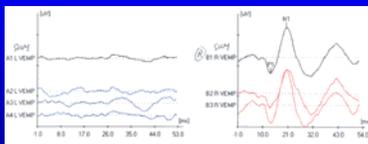


Good correlation between R-chair and VEMP
 Poor correlation between Caloric and VEMP.

Superior canal dehiscence (giant on one side)

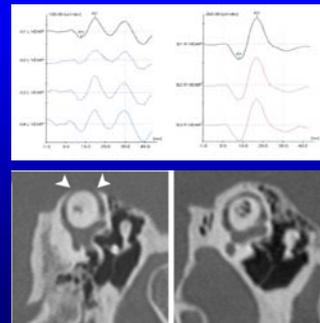

VEMP: Bottom Line

- Exciting emergent test
- Good test for bilateral loss (treatable by PT)
- Good test for SCD -- not treatable with PT
- Bad test for vestibular neuritis (because inferior nerve not affected in most VN)

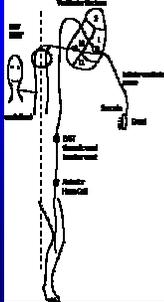


Rotatory Chair Testing


- Sinusoidal rotation in a chair over a spectrum of frequencies
- Measure gain and phase, compare with normal.



Normal Rotation Test

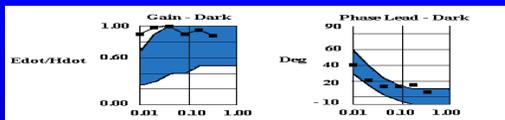

Rotation test after Gentamicin

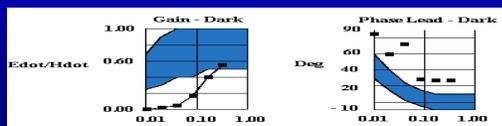

Rotatory Chair Testing Bottom Line

- Definitive test for bilateral vestibular loss
- Not very good for anything else


Moving Platform Posturography (MVP)

- Measure sway on a platform that can rotate about ankles and translate.
- 6 different sensory tests
- numerous "movement" tests measuring latency and strength of reactions



MVP for Malingers

- Six "sensory tests"--> gradient of difficulty
- Maligner tries to "fail" test, and adjusts sway to appear very unsteady on all tests
- Maligner fails easy tests.
- Examiner must not tell subject how to behave.
- Cevette algorithm -- linear discriminant score



MVP: Bottom Line

- Abnormal in conditions with poor balance (about as useful as the Romberg, which takes 10 seconds to do)
- Good test for malingerers – very useful.
- Bad test for diagnosis -- no diseases detected other than malingering



Summary – what you can learn from these tests

- ENG -- unilateral loss, bilateral loss (?)
BPPV
- VEMP test – unilateral loss, otolith disease, SCD
- Rot-chair -- bilateral loss
- Posturography -- malingering

More details

[The Handbook of Balance Testing](#)
(Ed. Jacobson and Newman), Mosby,
1992

www.dizziness-and-balance.com